

Supplementary Figure

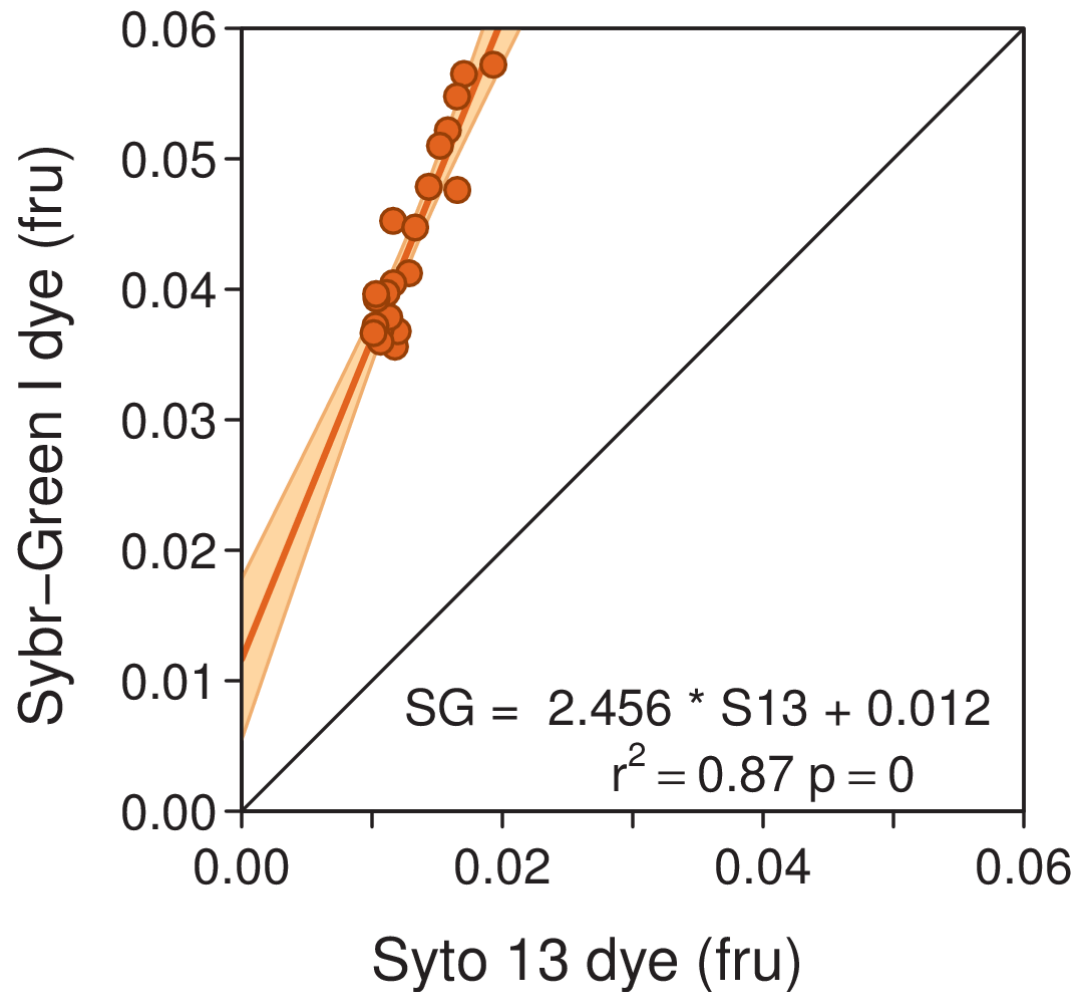


Fig. S1. Empirical calibration used to transform nucleic acid fluorescence in samples stained with Syto 13 to Sybr-Green I values in order to compare the 2002-2012 decadal mean and the 2012 experimental values shown in Fig. 1.