



Nano-mole scale sequential signal assignment by 1 H-detected protein solid-state NMR

Item Type	Article
Authors	Wang, Songlin;Parthasarathy, Sudhakar;Xiao, Yiling;Nishiyama, Yusuke;Long, Fei;Matsuda, Isamu;Endo, Yuki;Nemoto, Takahiro;Yamauchi, Kazuo;Asakura, Tetsuo;Takeda, Mitsuhiro;Terauchi, Tsutomu;Kainosho, Masatsune;Ishii, Yoshitaka
Citation	Wang S, Parthasarathy S, Xiao Y, Nishiyama Y, Long F, et al. (2015) Nano-mole scale sequential signal assignment by 1 H-detected protein solid-state NMR . Chem Commun 51: 15055–15058. Available: http://dx.doi.org/10.1039/c5cc04618a .
Eprint version	Post-print
DOI	10.1039/c5cc04618a
Publisher	Royal Society of Chemistry (RSC)
Journal	Chemical Communications
Rights	Archived with thanks to Royal Society of Chemistry (RSC);This file is an open access version redistributed from: http://europepmc.org/articles/pmc4589527?pdf=render
Download date	2024-02-28 00:21:55
Link to Item	http://hdl.handle.net/10754/594287



HHS Public Access

Author manuscript

Chem Commun (Camb). Author manuscript; available in PMC 2016 October 18.

Published in final edited form as:

Chem Commun (Camb). 2015 October 18; 51(81): 15055–15058. doi:10.1039/c5cc04618a.

Nano-mole Scale Sequential Signal Assignment by ^1H -Detected Protein Solid-state NMR using Ultra-Fast Magic-Angle Spinning and HIGHLIGHT Spectral Editing

Songlin Wang^a, Sudhakar Parthasarathy^a, Yiling Xiao^a, Yusuke Nishiyama^{c,d}, Fei Long^a, Isamu Matsuda^a, Yuki Endo^c, Takahiro Nemoto^c, Kazuo Yamauchi^{e,f}, Tetsuo Asakura^g, Mitsuhiro Takeda^h, Tsutomu Terauchiⁱ, Masatsune Kainosho^{h,j}, and Yoshitaka Ishii^{a,b}

Yoshitaka Ishii: yishii@uic.edu

^aDepartment of Chemistry, University of Illinois at Chicago, Chicago, IL 60607 Tel: 312-413-0076

^bCenter for Structural Biology, University of Illinois at Chicago, Chicago, IL 60607 Tel: 312-413-0076

^cJEOL RESONANCE Inc., 3-1-2 Musashino, Akishima, Tokyo 196-8558, Japan

^dRIKEN CLST-JEOL collaboration center, Yokohama, Kanagawa 230-0045, Japan

^eNuclear Magnetic Resonance Core Lab., King Abdullah University of Science and Technology, Thuwal 23955-6900, Saudi Arabia

^fSchool of Science and Technology, Nazarbayev University, Astana, Kazakhstan

^gDepartment of Biotechnology, Tokyo University of Agriculture and Technology 2-24-16, Nakacho, Koganei, Tokyo 184-8588, Japan

^hStructure Biology Research Center, Graduate School of Science, Furocho, Chikusa-ku, Nagoya University, Nagoya, Japan 464-8601

ⁱSAIL Technologies Co., Inc., 1-40 Suehiro-cho 1-chome, Tsurumi-ku, Yokohama, Kanagawa, Japan 230-0045

^jCenter for Priority Areas, Tokyo Metropolitan University, Tokyo 192-0397, Japan

Abstract

We present a 3D ^1H -detected solid-state NMR (SSNMR) approach for main-chain signal assignments of 10–100 nmol of fully protonated proteins using ultra-fast magic-angle spinning (MAS) at ~80 kHz with a novel spectral-editing method, which permits drastic spectral simplification. The approach offers ~110 fold time saving over a traditional 3D ^{13}C -detected SSNMR approach.

^{13}C high-resolution solid-state NMR (SSNMR) spectroscopy has been a powerful tool to analyze protein structures of amyloid, membrane-bound, or nano-crystalline proteins, for

Correspondence to: Yoshitaka Ishii, yishii@uic.edu.

Electronic Supplementary Information (ESI) available: [detailed protocols for the NMR experiments, including the pulse sequences used]. See DOI: 10.1039/b000000x/

which X-ray crystallography has been traditionally ineffective. However, limited sensitivity and resultant requirements of large sample amount have been a major bottleneck in traditional ^{13}C -detected SSNMR analysis of proteins for spectral assignment and structural analysis. A traditional ^{13}C 2D-3D SSNMR analysis has typically required 0.2–1 μmol of ^{13}C - and ^{15}N -labeled samples for signal assignments. ^1H indirect detection was introduced to ^{13}C and ^{15}N high-resolution SSNMR about a decade ago for sensitivity enhancement.^{1–4} The recent introduction of high-level deuteration and partial back-exchange of amide ^1H (10–20%) has greatly improved the ^1H resolution in protein SSNMR,^{5, 6} offering a practical protocol for ^1H -detected protein SSNMR. However, the sensitivity in the method has been limited by a gross loss of ^1H signals from amide sites (80–90%) due to deuteration. ^1H -detected ^{13}C SSNMR for a fully protonated protein at fast MAS (40–60 kHz) has offered signal assignments for proteins.^{7, 8} However, this method is still hampered by relatively broad ^1H line widths (0.3–1 ppm); the resolution is generally insufficient even for small proteins. Recent studies described ^1H indirect detection at a spinning frequency of 60 kHz, resulting in resolved amide ^1H resonances for fully deuterated proteins with fully back-exchanged amide ^1H .^{9, 10} Although those studies demonstrated higher ^1H resolution (0.1 ppm) and the feasibility of main-chain sequential assignments for micro-crystalline samples, these analyses using 3D SSNMR typically require 2–4 mg or 0.1–0.5 μmol of isotope-labeled protein samples, preparation of which can be still prohibitive for many proteins of biological interest. The limited sensitivity is presumably attributed to inefficient polarization transfer from amide ^1H to remote ^{13}C nuclei and many polarization transfer steps. Also, assignments from ^1H -detected 3D SSNMR is not so straightforward since the limited resolution in ^1H dimension typically causes spectral overlapping. Equally importantly, it has been difficult to achieve a net sensitivity gain by ^1H -detected ($N+1$)-dimensional SSNMR over a corresponding N -dimensional ^{13}C direct detected SSNMR without employing deuteration.¹¹ In this work, we present a novel approach for streamlining main-chain assignments of fully protonated proteins by ^1H -detected high-field SSNMR under ultra-fast MAS (UFMAS) at 80 kHz. Then, we show that main-chain assignments are feasible from a small set of 3D data with minimal sample requirements (10–100 nmol) by a combination of ^1H -detected SSNMR under UFMAS, a high field, paramagnetic doping, and a novel spectral editing. Our approach establishes advantage of ^1H indirect detection method over traditional ^{13}C direct detection for concurrent improvement in sensitivity and resolution for fully protonated proteins for the first time. The new approach collectively enhances sensitivity by 30–100 fold over a traditional moderate-field ^{13}C SSNMR approach.

Fig. 1a shows ^1H -detected 2D $^1\text{H}/^{15}\text{N}$ correlation SSNMR spectrum of a micro-crystalline GB1 sample that was uniformly ^{13}C - and ^{15}N -labeled except for lysine residues (Lys-reverse-labeled) under UFMAS at 80 kHz. $^{15}\text{N}/^1\text{H}$ correlations were observed for all the ^{15}N - ^1H groups of 56-residues GB1, except for 6 unlabeled lysine residues and 2 residues in the loop region (Ala-23 and Asp-47) (the sequence in Fig. 1c). The line widths of the resolved amide ^1H resonances in Fig. 1a are 0.21 ± 0.03 ppm. A corresponding 2D $^{15}\text{N}/^1\text{H}$ spectrum collected under MAS at 50 kHz (see Fig. S4) showed ^1H widths of 0.3–0.4 ppm, which are not sufficient to resolve individual lines even for a small protein.

This demonstrates drastic ^1H resolution improvements by a factor of 1.5–2 under UFMAS at 80 kHz.

With the excellent resolution, our next step is sequential assignments by ^1H -detected 3D experiments. Although a few previous studies reported sequential signal assignments of fully protonated proteins by ^1H -detected SSNMR,^{8, 12} main-chain signal assignments by ^1H -detected SSNMR have largely relied on spectral resolution in the ^1H dimension in 3D correlation spectra such as those obtained in CANH and CA(CO)NH experiments. In such experiments, nearly complete resolution is needed in a 2D $^{15}\text{N}/^1\text{H}$ chemical-shift correlation spectrum to achieve unambiguous sequential assignments. Due to spectral overlap, however, for many proteins it is not straightforward to establish starting points for sequential assignments with unambiguous assignments over a long protein sequence.

As an effective approach to address the spectral overlap problem in ^1H -detected SSNMR and to establish multiple starting points, here we introduce an approach called *HIGHLIGHT* (HIGH-speed-spinning-optimized Labeled-residue-IGNited Hetero-nuclear Total spectral quenching), which enables selective observation of residues adjacent to unlabeled residues in a reverse-labeled protein. For this purpose, we specifically designed a ^{13}CO – ^{15}N frequency-selective REDOR (fsREDOR) scheme,^{13, 14} which selectively quenches signals of ^{15}N bonded to ^{13}CO under UFMAS by selectively “recoupled” ^{13}CO – ^{15}N dipolar coupling (for details, see the Experimental section and Fig. S1). As the residues “highlighted” by this method are often varied in their amino acid types, spectral assignments are more straightforward than in selective amino acid labeling. In Fig. 1 (a, b), we compare 2D $^{15}\text{N}/^1\text{H}$ correlation spectra for a Lys-reverse-labeled micro-crystalline GB1 sample without (a) or with (b) *HIGHLIGHT* ^{13}CO – ^{15}N REDOR. By contrast, in the highlighted spectrum in (b), signals from six residues (Leu-5, Thr-11, Gly-14, Val-29, Gln-32, and Thr-51; residues in magenta in Fig. 1c) following lysine residues (Lys-4, -10, -13, 28, -31, and -50) can be observed clearly, beside the side-chain signal from ^{15}N – ^1H from Trp-43, which can be discriminated in the 2D CA(N)H experiment depicted in (d). The spectra in (a) and (b) were obtained only in 10 min and 20 min respectively by ^1H detection and additional sensitivity enhancement with paramagnetic-assisted condensed data collection (PACC) method,¹⁵ which employs short recycle delays of 0.3–1 s in the following experiments by taking advantage of short ^1H T_1 values in the presence of a paramagnetic dopant (~20 mM Cu-EDTA). In Fig. 1d, we show an overlay of ^1H -detected 2D CA(N)H correlation spectra without (blue) and with (red) selective dephasing due to ^{13}CO – ^{15}N dipolar coupling. It is obvious that only the residues following unlabeled lysine emerged in the *HIGHLIGHT* spectrum. In *HIGHLIGHT* REDOR, the intensities of the quenched residues were reduced to 0–12%, whereas 43–65% of the signals remained for highlighted residues in which ^{15}N groups were not directly bonded to ^{13}CO . Although a similar spectral-editing approach using “afterglow” spectroscopy has been proposed,¹⁶ this method only suppresses signals for non-target residues to ~1/3 of their initial values, leaving substantial background signals. Unlike other experiments designed for a low spinning speed (~13 kHz),^{14, 16} the *HIGHLIGHT* approach is effective under UFMAS, which is essential for an improvement in sensitivity by ^1H detection. Unlike amino-acid-selective labeling, the *HIGHLIGHT* approach offers excellent spectral dispersion from diverse amino acid types. Except for the

that in addition to 50- to 100-fold time-saving by the PACC method and a high-magnetic field, ^1H -detected SSNMR under UFMAS at 80 kHz further speeds up main-chain assignments by two orders of magnitude over traditional ^{13}C -detected 3D SSNMR. It should be noted that standard ^{13}C -detected correlations such as 3D CONCA typically require even more time than ^{13}C -detected 3D HNCA with an additional polarization transfer step. With the advantage, it is now feasible to complete assignments by a small set of 3D data and structural analysis for a 10–100 nmol of a fully protonated protein micro-crystalline sample unlike previous studies using fast MAS at ~ 60 kHz.

At the end, we demonstrate preliminary data showing that this HIGHLIGHT approach allows one to extend the advantage of ^1H -detected SSNMR under UFMAS to heterogeneous non-crystalline proteins of biological importance. For heterogeneous proteins such as amyloid fibrils, ^1H resolution is generally limited. Although ^1H -detected SSNMR showed promise in a recent study of deuterated $\text{A}\beta(1-40)$ amyloid fibers for assignments of relatively resolved spectral regions involving Gly¹⁹, a strategy of assignments by ^1H -detected SSNMR for heterogeneous proteins has been lacking particularly when the resonances are congested. In particular, sequential assignments are practically impossible when several residues having the same amino-acid type coexist in similar secondary structures. Figure 4 shows our preliminary data of 2D $^{13}\text{C}_\alpha/^{15}\text{N}$ projection spectra of 3DCANH data (a) with and (b) without HIGHLIGHT REDOR for amyloid fibrils of $\text{A}\beta(1-42)$ that is valine reverse ^{13}C - and ^{15}N -labeled (i.e. uniformly labeled except for valine). In (a), only 5 signals following valine residues are clearly resolved with spectral editing by the HIGHLIGHT approach, despite the nominal sample amount (~ 0.5 mg). In contrast, the 2D $^{13}\text{C}_\alpha/^{15}\text{N}$ projection in (b) shows substantial spectral overlapping. Indeed, in our attempt of traditional ^{13}C -detected 3D sequential assignments for 2 mg of uniformly ^{13}C - and ^{15}N -labeled $\text{A}\beta(1-42)$ fibril, all the valine $^{13}\text{C}_\alpha$ and ^{15}N resonances overlap around the same spectral region (data not shown). Thus, tracing the signals for valine and the residues following valine was not possible in a traditional ^{13}C -detected 3D SSNMR approach. The approach presented here offers a new avenue to achieve spectral resolution and assignments for residues following selected unlabeled residues as re-starting points of sequential assignments with a minimal quantity of the amyloid protein of ~ 100 nmol or less. Although the ^1H resolution for the amyloid protein sample is limited (^1H line widths ~ 0.9 ppm) due to its inherent structural heterogeneity (Fig. S5a–c), our data clearly suggest that spectral editing by the HIGHLIGHT approach and ^1H -detected SSNMR offer excellent means to assign unresolved resonances in sequential assignments with greatly enhanced sensitivity and resolution.

In conclusion, we demonstrated a general approach to achieve main-chain spectral assignments for a nominal quantity of a fully protonated protein sample by implementing combined use of ^1H detection under UFMAS at 80 kHz, PACC, and high-field SSNMR for the first time. First, we demonstrated that ^1H -detected SSNMR using the HIGHLIGHT approach could be highly effective for main-chain assignments for reverse-labelled proteins. Second, we experimentally demonstrated that ^1H indirect detection in 2D–3D SSNMR experiments notably improved sensitivity and resolution over traditional ^{13}C -direct detection in the corresponding 1-2D experiments. The approach does not require a high-level of ^2H -labeling, which can be cumbersome as it generally limits expression yield. Lastly, the very

high sensitivity achieved through a combination of high field SSNMR, PACC approach, and ^1H -detection using UFMAS at 80 kHz opens the door to nanomolar-scale SSNMR for main-chain signal assignments and conformation analysis of fully protonated proteins.

All SSNMR experiments were performed on a Bruker Avance III 750MHz spectrometer at the UIC Center for Structural Biology using a JEOL 1 mm $^1\text{H}/^{13}\text{C}/^{15}\text{N}/^2\text{H}$ quad-resonance MAS probe. The details of the experiments and the pulse sequences used for Fig. 1–4 are listed in the ESI (Fig. S1–3).

Supplementary Material

Refer to Web version on PubMed Central for supplementary material.

Acknowledgments

This study was supported primarily from the U.S. National Science Foundation (CHE 957793 and CHE 1310363) for YI. The instrumentation of the 750 MHz SSNMR at UIC was supported by an NIH HEI grant (1S10 RR025105). The preparation of A β (1–42) fibril sample was supported by an NIH RO1 grant (9R01GM098033) for YI.

References

1. Ishii Y, Tycko R. *J Magn Reson.* 2000; 142:199–204. [PubMed: 10617453]
2. Ishii Y, Yesinowski JP, Tycko R. *J Am Chem Soc.* 2001; 123:2921–2922. [PubMed: 11456995]
3. Paulson EK, Morcombe CR, Gaponenko V, Dancheck B, Byrd RA, Zilm KW. *J Am Chem Soc.* 2003; 125:15831–15836. [PubMed: 14677974]
4. Schnell I, Saalwachter K. *J Am Chem Soc.* 2002; 124:10938–10939. [PubMed: 12224915]
5. Chevelkov V, Rehbein K, Diehl A, Reif B. *Angew Chem Int Edit.* 2006; 45:3878–3881.
6. Reif B. *J Magn Reson.* 2012; 216:1–12. [PubMed: 22280934]
7. Zhou DH, Shah G, Cormos M, Mullen C, Sandoz D, Rienstra CM. *J Am Chem Soc.* 2007; 129:11791–11801. [PubMed: 17725352]
8. Marchetti A, Jehle S, Felletti M, Knight MJ, Wang Y, Xu ZQ, Park AY, Otting G, Lesage A, Emsley L, Dixon NE, Pintacuda G. *Angew Chem Int Edit.* 2012; 51:10756–10759.
9. Knight MJ, Webber AL, Pell AJ, Guerry P, Barbet-Massin E, Bertini I, Felli IC, Gonnelli L, Pierattelli R, Emsley L, Lesage A, Herrmann T, Pintacuda G. *Angew Chem-Int Edit.* 2011; 50:11697–11701.
10. Barbet-Massin E, Pell AJ, Retel JS, Andreas LB, Jaudzems K, Franks WT, Nieuwkoop AJ, Hiller M, Higman V, Guerry P, Bertarello A, Knight MJ, Felletti M, Le Marchand T, Kotelovica S, Akopjana I, Tars K, Stoppini M, Bellotti V, Bolognesi M, Ricagno S, Chou JJ, Griffin RG, Oschkinat H, Lesage A, Emsley L, Herrmann T, Pintacuda G. *J Am Chem Soc.* 2014; 136:12489–12497. [PubMed: 25102442]
11. Wang S, Parthasarathy S, Xiao Y, Nishiyama Y, Endo Y, Nemoto T, Matsuda I, Long F, Yamauchi K, Asakura T, Takeda M, Terauchi T, Kainosho M, Ishii Y. *Plos One.* 2015; 10:e0122714. [PubMed: 25856081]
12. Zhou DH, Shea JJ, Nieuwkoop AJ, Franks WT, Wylie BJ, Mullen C, Sandoz D, Rienstra CM. *Angew Chem Int Edit.* 2007; 46:8380–8383.
13. Jaroniec CP, Tounge BA, Herzfeld J, Griffin RG. *J Am Chem Soc.* 2001; 123:3507–3519. [PubMed: 11472123]
14. Traaseth NJ, Veglia G. *J Magn Reson.* 2011; 211:18–24. [PubMed: 21482162]
15. Wickramasinghe NP, Parthasarathy S, Jones CR, Bhardwaj C, Long F, Kotecha M, Mehboob S, Fung LWM, Past J, Samoson A, Ishii Y. *Nature Methods.* 2009; 6:215–218. [PubMed: 19198596]
16. Banigan JR, Gayen A, Traaseth NJ. *J Biomol NMR.* 2013; 55:391–399. [PubMed: 23539118]

17. Shen Y, Delaglio F, Cornilescu G, Bax A. *J Biomol NMR*. 2009; 44:213–223. [PubMed: 19548092]
18. Schmidt HLF, Sperling LJ, Gao YG, Wylie BJ, Boettcher JM, Wilson SR, Rienstra CA. *J Phys Chem B*. 2007; 111:14362–14369. [PubMed: 18052145]
19. Linser R, Dasari M, Hiller M, Higman V, Fink U, del Amo JML, Markovic S, Handel L, Kessler B, Schmieder P, Oesterhelt D, Oschkinat H, Reif B. *Angew Chem Int Edit*. 2011; 50:4508–4512.

Author Manuscript

Author Manuscript

Author Manuscript

Author Manuscript

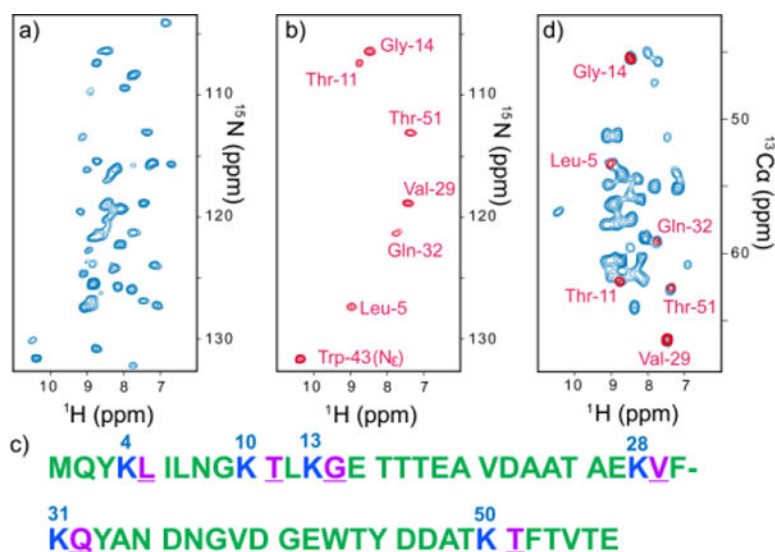


Fig. 1. (a, b) 2D ^1H -detected $^{15}\text{N}/^1\text{H}$ correlation spectra (a) without and (b) with HIGHLIGHT REDOR for the micro-crystalline sample of Lys-reverse-labeled GB1, along with the sequence shown in (c). (d) 2D ^1H -detected CA(N)H correlation spectra (blue) without and (red) with HIGHLIGHT REDOR, for the same sample. The sample was doped with 20 mM Cu-EDTA. The data were collected with recycle delays of 1 s at a spinning speed of $80,000 \pm 5$ Hz. The dephasing time due to $^{13}\text{CO}-^{15}\text{N}$ for HIGHLIGHT REDOR was 4.2 ms. The pulse sequences for the HIGHLIGHT experiments used for (b, d) are shown in Fig. S2 and S3.

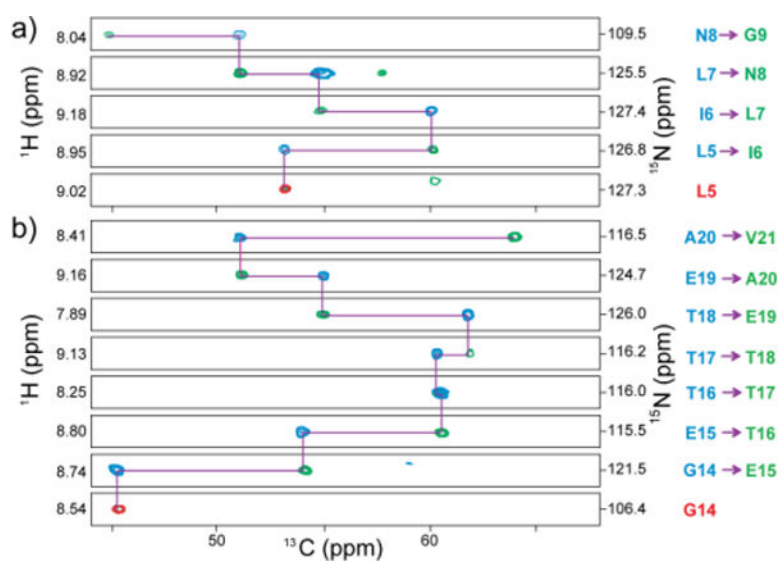
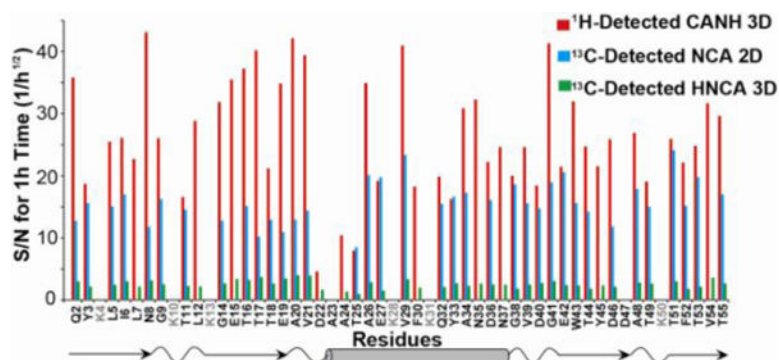


Fig. 2. Overlaid 3D strip plots for sequential assignments from (a) Leu-5 through Gly-9 and (b) Gly-14 through Asp-22 for a micro-crystalline sample of Lys-reverse-labeled GB1 protein obtained by 3D CANH (green), CA(CO)NH (blue), and 3D CANH with 4.2 ms HIGHLIGHT REDOR mixing data (red). The recycle delays were 0.3 s, 0.4 s, and 1 s for 3D CANH, 3D CA(CO)NH, and 3D CANH with HIGHLIGHT REDOR, respectively. All experiments were performed at a MAS spinning speed of 80 kHz with ~0.5 mg of sample. The total experimental times were 20 min for 3D CANH, 3.7 h for 3D CA(CO)NH, and 1 h for 3D CANH with HIGHLIGHT REDOR (for details, see the Experimental section and Fig. S2).

**Fig. 3.**

A comparison of signal-to-noise (S/N) ratios of 2D slices from ¹H-detected 3D CANH correlation (red bars), ¹³C-detected 2D NCA correlation (blue bars), and ¹³C-detected 3D HNCA correlation (green bars) of the GB1 sample. All the ratios were normalized to an experimental times of 1 h. The S/N ratios were normalized to the root-square of the experimental time. The secondary structures at the bottom were obtained from a published structure (PDB id: 2QMT).¹⁸ The S/N ratios for the overlapping peaks in the 2D NCA data are not shown. The average S/N ratios for an hour of the experimental time were 27.5, 15.2, and 2.6 for 3D CANH, 2D NCA, and 3D HNCA spectra, respectively.

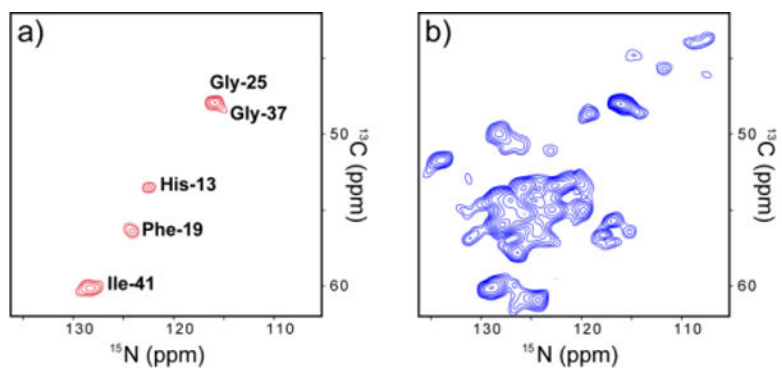


Fig. 4. 2D $^{13}\text{C}_\alpha/^{15}\text{N}$ projection spectra of 3D CANH data (a) with 4.2ms HIGHLIGHT REDOR mixing and (b) without the HIGHLIGHT REDOR for amyloid fibril of $\text{A}\beta(1-42)$ that is valine-reverse ^{13}C - and ^{15}N -labeled. Three 2D $^{13}\text{C}_\alpha/^{15}\text{N}$ slices from the 3D CANH spectrum are shown in Fig. S5. The experimental times are (a) 17.8 h and (b) 3.6 h.